Certificate of Analysis

LIQUILABS
Analytical services

Herbilabs
Herbilabs
Estonia
info@herbilabs.co.uk

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz

Verify Results Online

Sample Identification

Sample Name	BAC water
Batch Number	BW46-1001
Date Published	2026-11-23 10:16

Results for LIQ-0116

Stabilizers	Result	Unit	Uncertainty	Acceptable Range
Benzyl Alcohol Content Benzyl alcohol	0.98	%	[± 0.02]	0.9 - 1.1

Peptides	Result	Unit	Uncertainty	Acceptable Range
pH Determination pH determination	6.7		[± 0.1]	4.45 - 7

Microbiology	Result	Unit	Uncertainty	Acceptable Range
Total Aerobic Microbial Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	0	CFU/g	[±]	
Total Yeast and Mold Count USP <61>/Eur. Ph. 2.6.12. Plate Count Method	0	CFU/g	[±]	
Bacterial Endotoxin Chromgenic USP<85>/ Eur. Ph. 2.6.14. Bacterial Endotoxin Chromgenic Test	0.120	EU/vial	[± 0.002]	(RT) <= 0.25

Analysis Report

LIQUILABS
Analytical services

Sample Information

Injection Volume	: 1
Data File	: LIQ-0116__004.lcd
Method File	: Benzylalcohol v2.0.lcm
Date Acquired	: 13.10.2026 11:26:25

Chromatogram

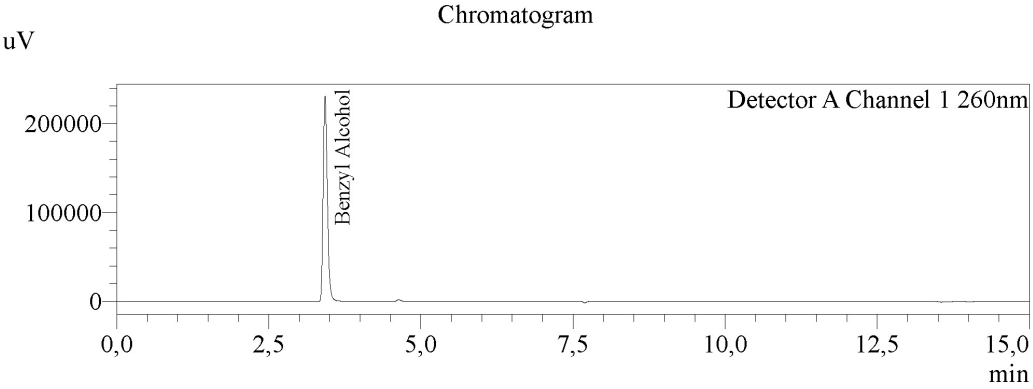

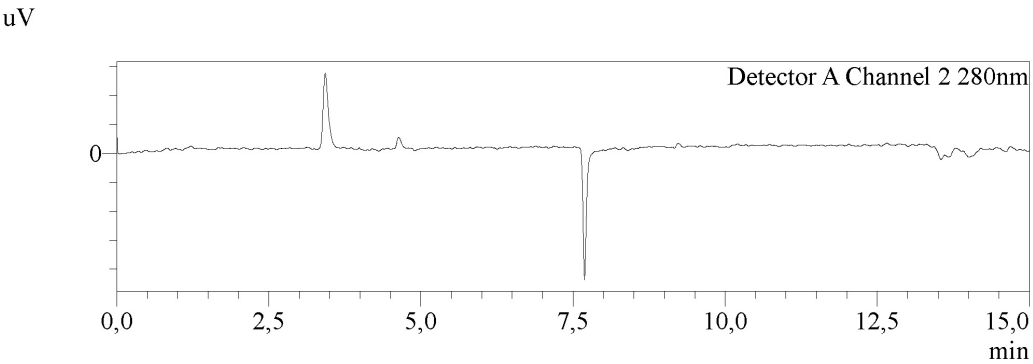

Peak Table

Detector A Channel 1 260nm

Peak#	Name	Ret. Time	Conc.	Unit	Area%
1	Benzyl Alcohol	3,422	0,985	% (m/m)	100,000
Total					100,000

Peak Table

Detector A Channel 2 280nm

Peak#	Name	Ret. Time	Conc.	Unit
1		3,426	0,000	
Total				

Liquilabs s.r.o. • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

Endotoxin Determination Report

File Information
Filename: C:\UVVis-Data\Data\File_261008_102802.vqud
Date/Time: 10/08/2026 11:02:59 AM

Instrument Information
Instrument Type: UV-1900 Series
Model (S/N): UV-1900i (A12536253123)

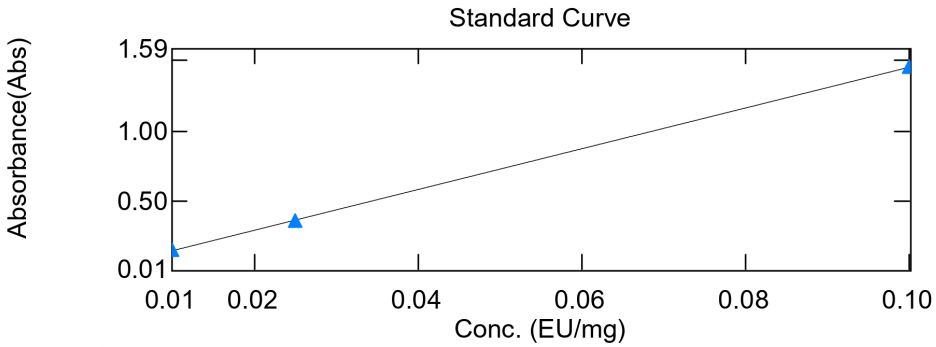

y = 14.5848 x - 0.00382298
r2 = 0.99998

	Sample Name	Conc	Raw_WL545.0	Dilution Rate
1	LYO-1059	0.245	0.1745	20.00
2	LYO-1141	0.152	0.1068	20.00
3	LYO-1064	2.017	0.7317	40.00
4	LYO-1144	1.618	0.5862	40.00
5	LYO-1066	0.109	0.0753	20.00
6	LYO-1067	0.110	0.0763	20.00
7	LYO-1172	0.121	0.0845	20.00
8	LYO-1058	2.143	0.7774	40.00
9	LYO-1060	2.769	1.0059	40.00
10	LYO-1061	0.104	0.0724	20.00
11	LYO-1098	0.172	0.1217	20.00
12	LIQ-0098	0.006	0.0863	1.00
13	LIQ-0116	0.012	0.1658	1.00
14	LYO-1143	0.574	0.0799	100.00

Liquilabs s.r.o. • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.
This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.

Liquilabs s.r.o. • Inovační 122 • 252 41 Zlatníky-Hodkovice • Czechia
Phone : +420 608 444 727 • Fax : • jan.galbavy@liquilabs.cz • www.liquilabs.cz